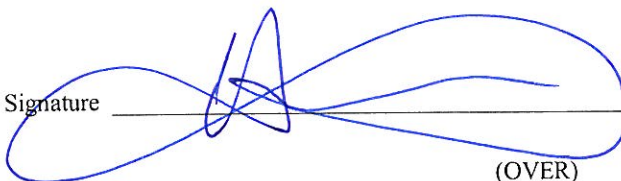


# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument  
State of Alaska

JUL 13 2010


Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130193 ✓
Name	James C. Gipson	ID#	4842 ✓
		Date	07/03/2010 ✓
A	Agency	Palmer Police Department	Phone # 745-4811
	Instrument Location	Palmer Police Department	
Alco S/N		718493 ✓	Target Value .084 ✓
			High Pressure 1300
B	Alco Test Values	.082 ✓	.084 ✓
		1 <sup>st</sup> Alco	2 <sup>nd</sup> Alco
Signature			
		(OVER)	


(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:


- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 27<sup>th</sup> day of July, 2010.

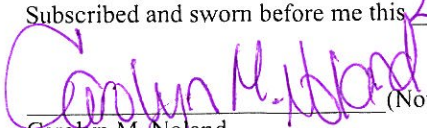  
Carolyn M. Noland  
Notary Public, State of Alaska  
Commission Expires with Office

(Notary Seal Stamp)



# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130193

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130193

JULY 03, 2010

OPERATOR'S NAME:

GIPSON/JAMES/C

OPERATOR'S NUMBER: 4842

SUBJECT'S LAST NAME:

VERIFICATION OF CAL

SUBJECT'S FIRST NAME/MI :

RJC60

O.L. #: 0123456

DEPT/AGENCY: PLM1

CASE/REPORT: 01-2345

TEST TYPE: U

ALCO TARGET VALUE: .084

ALCO S/N: 718493

--- BREATH ANALYSIS ---

.084 ADJUSTED FOR 29.73 in

ALCO TARGET .083 06:39

BLANK TEST .000 06:40

INTERNAL STANDARD VERIFIED 06:41

ALCO TV 29.75 in .082 06:41

BLANK TEST .000 06:41

SUBJECT SAMPLE .000 06:42

BLANK TEST .000 06:43

ALCO TV 29.73 in .084 06:43

BLANK TEST .000 06:44

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130193

JULY 03, 2010

TIME 06:45

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 01/08/09

HEATERS

SAMPLE CHAMBER: 48c

BREATH TUBE: 43c

BAROMETER: 29.73 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!"#\$%&'()\*+,-./0123456789:;<=>?@ABCDEFGHIJ  
KLMNOPQRSTUVWXYZ[\]^\_`abcdefghijklmnopqrstuvwxyz{|}~